

# FRESENIUS 2008K HEMODIALYSIS SYSTEM

# PREVENTIVE MAINTENANCE PROCEDURES

Part Number 507297 Rev. H

# FRESENIUS MEDICAL CARE NORTH AMERICA

800-227-2572 or 925-295-0200

Fresenius Medical Care North America 920 Winter St. Waltham, MA 02451

> Manufactured by: Fresenius USA, Inc. 2637 Shadelands Drive Walnut Creek, CA 94598

REGIONAL EQUIPMENT SPECIALIST:	



## FRESENIUS 2008K HEMODIALYSIS SYSTEM

## PREVENTIVE MAINTENANCE PROCEDURES

Part Number 507297 Rev. H

INCLUDING
PREVENTIVE MAINTENANCE CHECKLISTS
QUARTERLY/1000 HOUR AND ANNUAL/4000 HOUR

http://www.fmcna.com

Copyright © 2000 - 2012 Fresenius Medical Care North America



### **WARNINGS**

Shock hazard. Refer servicing to qualified personnel.

Failure to install, operate and maintain this equipment according to the manufacturer's instructions may cause patient or operator injury or death.

Never perform maintenance when a patient is connected to the machine. If possible, remove the machine from the treatment area when it is being serviced. Label the machine to ensure it is not accidentally returned to clinical use before the service work is completed. Always fully test the machine when maintenance is completed. Confirm dialysate conductivity and pH level before returning the machine to clinical use.



## PREVENTIVE MAINTENANCE PROCEDURES TABLE OF CONTENTS

1.0	INTRODU	UCTION	
1.1	TEST EQ	QUIPMENT AND SUPPLIES NEEDED	1
1.2		ING MODES	
1.3		PANEL CONTROLS	
1.4		RING FLUID VOLUMES	
2.0	QUARTE	RLY (1000 HOUR) PREVENTIVE MAINTENANCE	7
	2.1	FILTERS AND O-RINGS	
	2.2	DIASAFE® FILTER (IF APPLICABLE)	
	2.3	CHECK VALVES	10
	2.4	HIGH VOLTAGE AC CONNECTIONS	
	2.5	UF PUMP	
	2.6	CONDUCTIVITY	
	2.7	TEMPERATURE	
	2.8	LEVEL DETECTOR	
	2.9	ALARM AND PRESSURE HOLDING TESTS	
	2.10	POWER FAILURE ALARM	19
	2.11	BLOOD PUMP ROTOR INSPECTION	
	2.12	FINAL CHECKS	
3.0		_ (4000 HOUR) PREVENTIVE MAINTENANCE	23
	3.1	FILTERS AND O-RINGS	23
	3.2	PRE-UF PUMP FILTER	
	3.3	CHECK VALVES	
	3.4	DEAERATION RESTRICTOR	
	3.5	DIASAFE® FILTER (IF APPLICABLE)	
	3.6	DIAPHRAGM PUMPS	
	3.7	HEATER ELEMENT	
	3.8	HIGH VOLTAGE AC CONNECTIONS	
	3.9	DEAERATION MOTOR BRUSHES	
	3.10	INLET WATER PRESSURE REGULATOR	
	3.11	ONLINE CLEARANCE TEST (IF APPLICABLE)	
	3.12 3.13	DEAERATION AND LOADING PRESSURE	
	3.13	FLOW RELIEF PRESSURECONCENTRATE AND BICARB PUMPS	33 21
	3.14		
	3.15	UF PUMPCONDUCTIVITY	
	3.10	TEMPERATURE	
	3.17	VOLT HI LO DETECT	
	3.19	BLOOD LEAK AND DIMNESS	
	3.20	ARTERIAL, VENOUS AND TRANSMEMBRANE PRESSURE	36
	3.21	DIALYSATE FLOW	30
	3.22	HEPARIN PUMP	
	3.23	BLOOD PUMP	
	3.24	LEVEL DETECTOR	
	3.25	ALARM AND PRESSURE HOLDING TESTS	
	3.26	RINSE CHECKS	
	3.27	BATTERY AND POWER FAILURE ALARM	
	3.28	BLOOD PRESSURE MODULE	47
	3.29	FINAL CHECKS	51
4.0	REBUII F	DING THE DIAPHRAGM PUMPS	
	4.1	REBUILDING THE ULTRAFILTRATION PUMP	
	4.2	REBUILDING THE CONCENTRATE AND BICARBONATE PUMPS	
	4.3	TESTING CONCENTRATE AND BICARBONATE PUMPS	
PRF		MAINTENANCE CHECKLIST QUARTERLY/1000 HOUR	
		MAINTENANCE CHECKLIST ANNIHAL //1000 HOUR	



### **NOTE**

This document is written for Fresenius 2008K Hemodialysis Systems using software versions 2.16 or later.



#### 1.0 INTRODUCTION

Preventive Maintenance for the Fresenius 2008K Hemodialysis System is simple and straightforward. Maintenance is performed in only two intervals: Quarterly or after 1000 hours of operation, and annually or after 4000 hours of operation. The maintenance procedures have been devised to require a minimum of time while ensuring that the machine is maintained in optimum operating condition.

Included in the Preventive Maintenance procedures are tests to verify normal machine operation. Should the machine fail to pass any of these tests, repair or recalibrate as needed, then repeat the tests until the specifications are met before returning the machine to service.

Checklists are provided in the back of this manual to record the work done. Make copies of these checklists as needed. Your initials on the checklist certifies that each procedure has been completed and that the machine is performing according to the specifications given.

#### 1.1 TEST EQUIPMENT AND SUPPLIES NEEDED

A number of small parts must be available to perform the Preventive Maintenance. Fresenius part number 190098 is a kit of the parts needed, except for the 9-Volt battery that must be replaced during the annual preventive maintenance. An NEDA 1604AC heavy-duty (alkaline type) battery is required. In addition, the following test equipment is needed:



**Warning!** All of the test equipment used must be maintained and calibrated regularly in accordance with NIST standards. In particular, the conductivity meter must meet the specifications given below. Failure to do so could result in injury or death to the patient or to the operator.



**Warning!** Disinfect the machine internally and externally and check all pressure transducer protectors for contamination before working on the machine.



- Fresenius Test Kit (Fresenius part number 150034), which contains two gauges with fittings and hoses for measuring loading pressure and deaeration pressure.
- Dialysate meter to measure dialysate pressure, temperature and conductivity at the ends of the dialysate lines. The meter must be capable of making pressure measurements from -250mmHg to +400mmHg with an accuracy of at least ±3mmHg. The temperature function of this meter must be accurate within 0.2°C from 20°C to 45°C and must be capable of measuring dialysate temperatures up to 85°C with an accuracy of at least ±4.0°C. The conductivity function of this meter must be accurate to within 0.1mS over a range of 12mS to 17mS at a temperature of 25°C.
- Stopwatch with a resolution to 0.01 second and an accuracy of 0.01% or better.
- Fresenius Buret, 25ml capacity with 0.1ml graduations (Fresenius part number 290104).
- Graduated cylinder: 1000ml capacity with a tolerance of 5.0ml at 1000ml or better.
- Syringe, 60cc capacity. Tolerance is not important; the syringe is not used for volume measurements.
- Tubing, 24" long (Fresenius part number 545325-10). Use on the tip of the Buret.
- Resistor Plug Set for OLC Testing (Fresenius part number 190168).

The following equipment is also required to test the blood pressure module:

- Test Device (Fresenius part number 370090). The Test Device contains two air chambers with calibrated volumes.
- Mercury manometer or equivalent pressure meter accurate to within 1mmHg at pressures up to 330mmHg.



#### 1.2 OPERATING MODES

The following preventive maintenance procedures contain instructions to place the 2008K into Dialysis Mode and Service Mode.

To place the machine in Service Mode, turn the machine power On and wait for the message Press CONFIRM for Service Mode to appear. Once it appears, press the [CONFIRM] key and the message will change to Machine in Service Mode. After the System Initializing process is complete, the machine will be in Service Mode.

If the [CONFIRM] key is not pressed when the Press CONFIRM for Service Mode message is on the screen, the screen will change and the message Machine in Dialysis Mode will appear. After the System Initializing process is complete, the machine will be in Dialysis Mode.



#### 1.3 FRONT PANEL CONTROLS

The front panel consists of two areas, the touch screen and the control panel. The touch screen is the area under the glass in the center of the front panel. The control panel surrounds the touch screen and it contains the membrane keys.

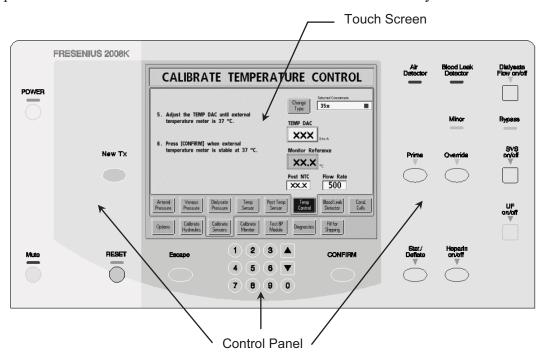


Figure 1 - 2008K Front Panel

#### **Control Panel Operation**

Throughout the preventive maintenance procedures, whenever a control panel key is to be pressed, the appropriate key name is surrounded by square brackets as in the following example:

Press the [CONFIRM] key and the screen will change.

In this example, the [CONFIRM] key on the control panel should be pressed.



#### **Touch Screen Operation**

The touch screen is designed to display information and is used to enter data. To select a button during a procedure, locate the button on the screen. Select a parameter for which data will be entered using the keys below the screen. Depending on the type of button, the screen will change. Data boxes are also displayed on the touch screen. The following describes the type of buttons and data boxes that will be encountered during the preventive maintenance process.

#### **Data Button**

A yellow data button is used to enter a measured volume or value. When the yellow area of the data button is touched, it will change to a darker yellow. The data can be changed using the [▲] or [▼] keys or the value can be entered using the number keys both on the control panel. Once the data is entered, press the [CONFIRM] key and the data button changes back to light yellow. The [Escape] key can be pressed when the data button is dark yellow to abort the data entry and return it to light yellow. The entered data does not get stored until the [CONFIRM] key is pressed.



Some data buttons will change the screen and the data entry will be performed on the new screen.

A gray data button means the button is not active and touching it will have no effect.

#### Screen Button

Blue rectangles on the touch screen are screen buttons. By touching the blue area of the screen button the display will either change to another screen or the selection of an option will change. A screen button is not active if it is gray.





#### Data Box

This type of box shows selected data or data the machine is measuring. During the preventive maintenance process this type of box is used to verify a value or selection.



FC3000	35x ■



#### 1.4 MEASURING FLUID VOLUMES

Several of the following procedures require measuring fluid volumes using graduated cylinders and laboratory burets. When making these measurements do the following:

- Make certain the container is clean and dry before collecting the fluid to be measured. Two drops of fluid are approximately 0.1ml, which is enough to affect the accuracy of critical measurements.
- Ensure that no items such as thermometers or tubing are allowed to come in contact with the fluid in the graduate. Such items will change the calibration of the graduate and affect the accuracy of measurements. Both the total volume indicated and the amount of fluid indicated by each increment on the graduated scale will be incorrect. For example, if a graduate is calibrated in 1ml increments, a piece of tubing in contact with the fluid will cause each increment to be *less* than 1ml, depending upon the total volume of the tubing that penetrates into the fluid.
- Surface tension causes the fluid to curve into a meniscus (See Figure 2). Measure the volume at the bottom of the meniscus curve as shown.

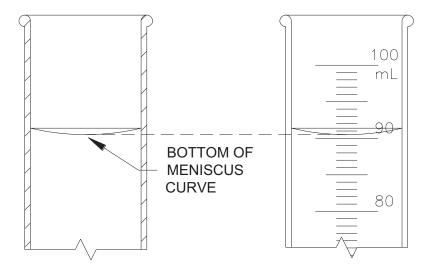


Figure 2. Meniscus Curve.



#### 2.0 QUARTERLY (1000 HOUR) PREVENTIVE MAINTENANCE

Perform the following Preventive Maintenance procedures every 3 months or 1000 hours of machine operation, whichever comes first. Make copies of the Quarterly Preventive Maintenance Checklist provided in the back of this manual and use them to record the maintenance done.

When performing an Annual Preventive Maintenance, do not perform the quarterly procedures below first. Go directly to Section 3 and perform the annual procedures described there. You will be referred back to this section to perform the quarterly procedures along with the annual procedures in the most efficient order.

While performing the following procedures, check the floor of the hydraulic unit and all surfaces for moisture that might indicate a leak. Locate and correct any leaks detected. Clean the floor of the hydraulic unit so that future leaks will be readily apparent. Also, check all electrical connectors that can be reached to be sure they are fully seated and there is no strain on the electrical cables.



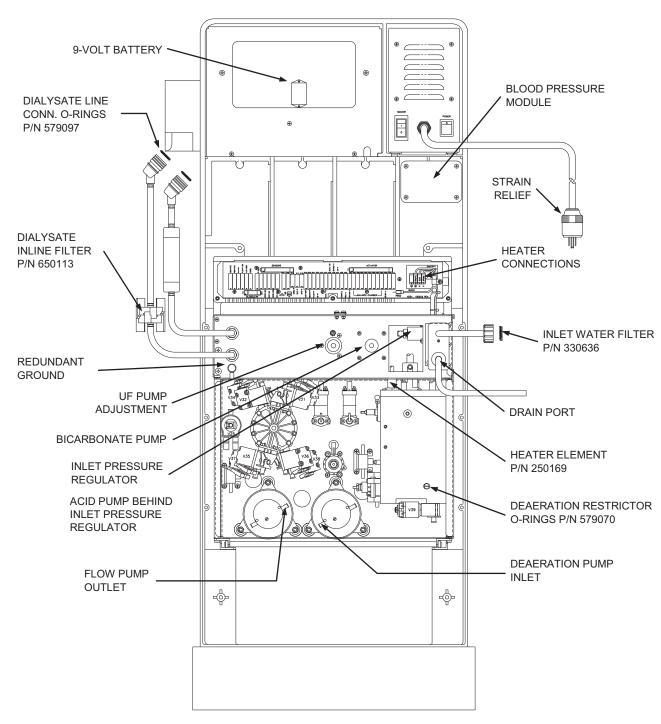


Figure 3. Fresenius 2008K Hemodialysis System, Rear View.



#### 2.1 FILTERS AND O-RINGS

Clean filters and replace O-rings as follows. Replace any filters that appear damaged or corroded.

1. Inlet Water Filter in the inlet connector of the water supply (See Figure 3, pg. 8).



**Warning!** After cleaning or replacing the inlet filter screen, disinfect the water inlet line as described in the Operator's manual and in accordance with your Unit Policy.



**Warning!** Do not use excessive O-ring lubricant, as silicone-gel can damage the hydraulic pressure transducers (P-DIAL and CFS).

2. Filters and O-rings in the Concentrate and Bicarbonate Connectors (See Figure 4). Replace all three O-rings in each connector.

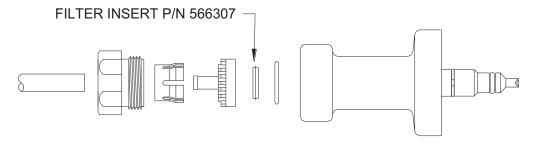


Figure 4. Concentrate and Bicarbonate Connector Assemblies.

- 3. Dialysate Inline filter (See Figure 3, pg. 8).
- 4. O-rings in the Dialysate Line Connectors (See Figure 3, pg. 8).



5. Pre-UF Pump Filter. Inspect the Pre-UF Pump filter for leaks or distortion. Replace the Pre-UF Pump Filter if leakage or distortion is found.



**Caution:** Do not attempt to disassemble the Pre-UF Pump Filter. If not properly reassembled, the Pre-UF Pump filter may leak. A leak in the hydraulic system at this location may affect the operation of the machine or cause fluid loss from the patient.

#### 2.2 DIASAFE® FILTER (IF APPLICABLE)

If the machine is equipped with a DIASAFE® or DIASAFE® PLUS filter system, replace the filter every 90 days (quarterly). After replacing the filter, perform either the automated test function or a manual pressure holding test AND then perform the DIASAFE® filter integrity test.



**Note:** If the machine is equipped with a DIASAFE<sup>®</sup> filter, replace its quick connector O-rings (Fresenius part number 579097) when replacing the filter.

#### 2.3 CHECK VALVES



**Caution:** If a check valve is replaced, ensure it is oriented correctly to allow fluid flow in the proper direction.

Inspect the UF Pump Output check valves (one at the UF pump and the other downstream at the UF Sample Port). Replace any that show signs of wear, damage or leaking.



#### 2.4 HIGH VOLTAGE AC CONNECTIONS



**Warning!** Dangerous high voltage is present at the connections accessed in this procedure when the machine is operating. Ensure the machine's power plug is disconnected from the wall outlet before proceeding.

- 1. Remove power from the machine then check and tighten the 8-pin heater connections on the distribution board (See Figure 3, pg. 8). Check heater block AC connections for signs of arcing or melting.
- 2. If applicable, inspect the power plug for loose or frayed wires. Ensure the strain relief is securely fastened.
- 3. Inspect the entire length of the power cord (from plug to strain relief) for nicks or cuts in the insulation and replace if necessary (Fresenius part number 150425).
- 4. Confirm that the strain relief is tightly secured to the power supply chassis.
- 5. At the strain relief, locate the black, white and green wires from the power cord (inside the power supply chassis). Follow the black and white wires to the main power switch. Attached to the main power switch are four (4) wires (2 black and 2 white). Look for loose connections, cracked insulation, and signs of overheating, such as discolored or melted insulation. Replace wires with power supply wire kit (Fresenius part number 190411).
- 6. Inspect the main power switch and verify that its operation is smooth (no grinding or sticky operation) and that the wires are not crossed.
- 7. With a digital multimeter, measure the resistance between the round (ground) pin on the power plug and the redundant ground terminal on the machine (See Figure 3, pg. 8). Verify that the resistance is less than 0.2 ohm. If the value is above 0.2 ohm, measure the internal resistance of your meter by shorting the leads together, then subtract this value from the resistance measured between the power plug ground pin and the redundant ground terminal on the machine to obtain the true ground resistance.



**Warning!** Do not operate the machine if the resistance is greater than 0.2 ohm. A shock hazard to operators and patients could exist.

8. Perform the electrical safety checks required by local codes, facility procedure and the Joint Commission on Accreditation of Healthcare Organizations.



#### 2.5 UF PUMP

Calibrate the UF Pump Volume (Refer to the 2008K Calibration Procedures – Fresenius part number 507296.)

#### 2.6 CONDUCTIVITY

Verify that the dialysate conductivity measured by the internal cell in the machine agrees with an external meter within 0.1mS/cm as follows:

- 1. Connect an external conductivity meter to the dialysate lines.
- 2. With the machine in Dialysis Mode and flow ON, compare the value shown on the external meter with the conductivity shown on the Display screen. They must be within 0.1mS/cm of each other.

#### 2.7 TEMPERATURE

Verify that the actual dialysate temperature measured by an external meter agrees with the display screen within 0.5°C at 37°C and 39°C as follows:

- 1. Connect the dialysate lines to an external meter.
- 2. Place the machine in Dialysis Mode with concentrate in the system. Clear any alarms.
- 3. Select the Temperature button. The button label will change to Temp. Setting. The value now displayed on this button is the temperature set point. Adjust the temperature set point to exactly 37.0 then press the [CONFIRM] key. The button will change back and now reads the actual temperature of the dialysate again. Wait until this value stabilizes. It will settle very close to the value set, depending upon inlet water temperature and other conditions.
- 4. After the temperature of the dialysate stabilizes, compare the temperature shown on the Temperature button with the temperature shown on the external meter connected to the dialysate lines. The two readings must be within 0.5° of each other.
- 5. Repeat steps 3 and 4 with the temperature set to 39.0°C. Verify that the actual temperature reported on the front panel display screen and the external meter is within 0.5° of each other after the temperatures stabilize again.



#### 2.8 LEVEL DETECTOR



**Caution:** In the following steps, the level detector must be removed from the machine cabinet. Before returning it to the cabinet, wipe the lower edge of the module and the level detector cabinet opening to remove any residual disinfecting agent. When installing the module screws do not use a power screwdriver.

#### **ALARM TEST**

- 1. Calibrate level detector (Refer to Section 3.2 of the 2008K Calibration Procedures Fresenius part number 507296).
- 2. Place the machine in Dialysis Mode and turn the blood pump ON. Insert a water filled venous chamber into the level detector and clear all alarms.
- 3. Position the Level Detector so you can watch the Channel 1 and Channel 2 LED's on the circuit board (See Figure 6 on page 15).
- 4. While watching the Channel 1 and Channel 2 LED's, remove the venous chamber to create a blood alarm and close the occlusion clamp. Verify that the Channel 1 LED lights first followed quickly by Channel 2.

#### OCCLUSION CLAMP TEST

- 1. Place a venous line into the closed occlusion clamp. Do not connect this line to the venous chamber in the level detector.
- 2. Place the lower end of the venous line below the occlusion clamp in a container of water positioned so that air escaping from the end of the line is easily seen.
- 3. Connect a syringe and a pressure gauge to the venous line above the occlusion clamp.
- 4. With the syringe, apply a pressure of at least 30psi (1550mmHg) to the venous line while watching the end of the venous line in the water.
- 5. Verify that no air escapes from the venous line, indicating that the clamp is fully occluding the line.



#### RELAY CONTACT TEST

A relay prevents the level up and level down membrane keys on the face of the level detector to function if they are pressed at the same time.

Various module configurations are available. Use the following information to select the correct method to use to check the relay contacts:

- Use Method 1 if LP450 has LED's D6 & D19 (See Figure 5)
- Use **Method 2** if LP450 does not have relay test LED's then locate a separate relay board LP1026 with test LED's D3 & D4 (See Figure 5).
- Use **Method 3** if LP1026 is present and does not have LED's D3 & D4 (See Figure 6).

#### Method 1:

- 1. With the machine in Dialysis Mode and the blood pump turned ON, insert a water filled venous chamber into the level detector and clear all alarms
- 2. Locate the relay test LED's D6 and D19 on the LP450 board.
- 3. To test the LED's, press the level down switch on the face of the level detector and verify that both LED's D6 and D19 light. The on-board air pump will also run. If both LED's light, proceed to step 4.



**Note:** If either LED doesn't light during the LED test (step 3), then the results of the Relay Contact Test (step 4) would be invalid. In this case use Method 3 instead.

While in alarm condition (clamp closed), attach the ground lead of a voltmeter to TP3 (ground) on the LP450 board. Measure the voltage on the solder side of pins 1 and 2 of X153 on the LP450 board. Verify that both pins are 0 volts. If voltage is present, the relay contacts are bad.

4. To test the relay contacts, remove the venous chamber to create a blood alarm and verify that both LED's D6 and D19 do <u>not</u> light when the level down switch is pressed. If either LED lights, the relay contacts are bad.



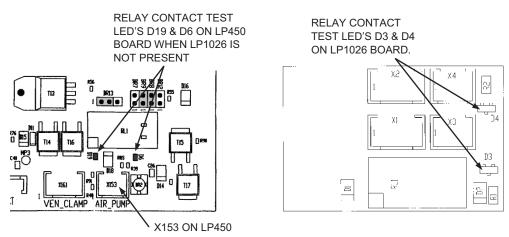


Figure 5 - Level Detector with Relay Contact Test LED's.

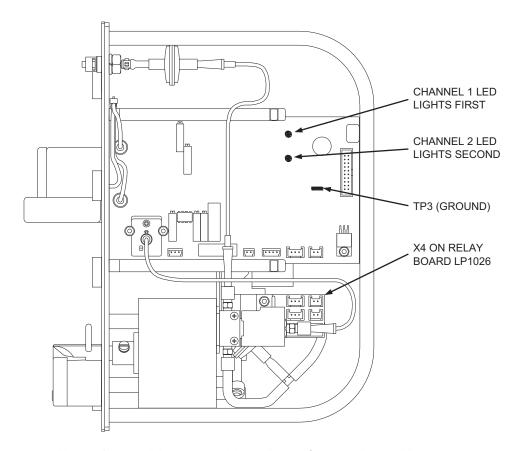


Figure 6 - Level Detector without Relay Contact Test LED's.



#### Method 2:

- 1. With the machine in Dialysis Mode and the blood pump turned ON, insert a water filled venous chamber into the level detector and clear all alarms.
- 2. Locate the relay test LED's D3 and D4 on the LP1026 board.
- 3. To test the LED's, press the level down switch on the face of the level detector and verify that both LED's D3 and D4 light. The on-board air pump will also run. If both LED's light, proceed to step 4.



**Note:** If either LED doesn't light during the LED test (step 3), then the results of the Relay Contact Test (step 4) would be invalid. In this case use Method 3 instead.

4. To test the relay contacts, remove the venous chamber to create a blood alarm and verify that both LED's D3 and D4 do <u>not</u> light when the level down switch is pressed. If either LED lights, the relay contacts are bad

#### Method 3:

- 1. With the machine in Dialysis Mode and the blood pump turned ON, insert a water filled venous chamber into the level detector and clear all alarms
- 2. Locate the solder side of X4 on the LP1026 (or X153 on the LP450).
- 3. Attach the ground lead of a voltmeter to TP3 (ground) on the LP450 board.
- 4. Test for 24 volts at X4 (X153) by pressing the level down switch on the face of the level detector and verify that both pins 1 and 2 on the solder side of X4 (X153) are 24 volts.
- 5. To test the relay contacts, remove the venous chamber to create a blood alarm and measure the voltage on the solder side of pins 1 and 2 of X4 (X153). Verify that both pins are 0 volts. If voltage is present, the relay contacts are bad.



#### 2.9 ALARM AND PRESSURE HOLDING TESTS

Verify the automatic alarms produce the responses shown in Table 1 and the machine passes the automatic pressure holding test as follows:

1. Place the dialysate lines in the shunt and close the door.



**Warning!** The use of a "test drip chamber" or "dummy drip chamber" <u>must never be used on the treatment floor</u>. It must only be used in a controlled technical environment.

- 2. Place a venous chamber filled with water in the holder on the level detector module.
- 3. Place the machine in Dialyze mode and start the blood pump. Clear all blood and water alarms.
- 4. Select the Test & Options button. On this screen press the Both Tests button. Press the [CONFIRM] key to start.
- 5. Observe the machine stepping through the following alarm tests and ensure that each alarm produces all of the responses shown in Table 1.



Table 1. Alarm Tests.

ALARM TEST	RESPONSE
Air Detector	<ol> <li>Red visual alarm</li> <li>Venous clamp closes</li> <li>Blood pump stops</li> </ol>
Blood Leak	<ol> <li>Red visual alarm</li> <li>Venous clamp closes</li> <li>Blood pump stops</li> </ol>
Arterial Pressure	Red visual alarm     Venous clamp closes     Blood pump stops
Venous Pressure	Red visual alarm     Venous clamp closes     Blood pump stops
TMP	Red visual alarm     Venous clamp closes     Blood pump stops
9-Volt Battery	Passes if battery voltage is greater than 7.0 volts under a load of $22\Omega$ .
Optical Detector	Lower venous alarm limit rises to 10mmHg causing a venous pressure alarm     Venous clamp closes     Blood pump stops
Temperature	Red visual alarm     Yellow visual bypass     Machine in Bypass mode (no flow through the dialysate flow indicator).
Conductivity	Red visual alarm     Yellow visual bypass     Machine in Bypass mode (no flow through the dialysate flow indicator).



- 6. When the tests shown in Table 1 are complete, the machine conducts a pressure holding test. When the test ends verify that the display screen reports TEST COMPLETE, indicating that all the tests were passed successfully. Press the [RESET] key.
- 7. Test the UF pump integrity as follows:
  - Pull the hydraulics out and remove the output tube from the UF pump.
  - Install a 24" tube (Fresenius part number 545325-10) to the empty output port. Route this tubing out the back of the machine so that it will not be kinked or pinched when the hydraulics is closed. Close the hydraulics and place the other end of tube into a collection container.
  - Conduct steps 1-6 again.
    - If the pressure holding test <u>fails</u>, refer to Section 4.1.
    - If the pressure holding test <u>passes</u>, disconnect the 24" tube and reconnect the original output tube to the UF pump.
- 8. Test the audible alarm as follows:
  - Place a piece of opaque paper inside the housing of the optical detector to simulate a line containing blood. Close the door of the optical detector.
  - Open the shunt door. Verify that the machine responds with an audible alarm. Press the [Mute] key and verify that the Mute lamp lights, and the audible tone stops.

#### 2.10 POWER FAILURE ALARM

Test the Power Failure alarm by turning the main power switch off on the back of the power supply with the machine powered on. Verify that the audible alarm sounds. If no audible alarm occurs, check/replace the 9-Volt battery.



#### 2.11 BLOOD PUMP ROTOR INSPECTION

Clean and inspect the arterial blood pump rotor assembly as follows:

- 1. Remove the blood pump rotor by opening the door, pulling out the crank lever and turning the rotor 90 degrees.
- 2. Clean the rollers with a cloth dampened only with water.
- 3. With the crank lever pulled out, locate and lubricate the crank lever retainer ball. See Figure 7 for assistance. If the crank lever is hard to pull out, replace the crank lever retainer assembly (Fresenius part number 564301).
- 4. Clean the inside of the blood pump housing with the damp cloth. Compressed air may be used if it is available.
- 5. Locate the four (4) tubing guides. See Figure 7 for assistance. If any of the four (4) tubing guides are missing, the rotor assembly needs to be replaced (Fresenius part number M30990).

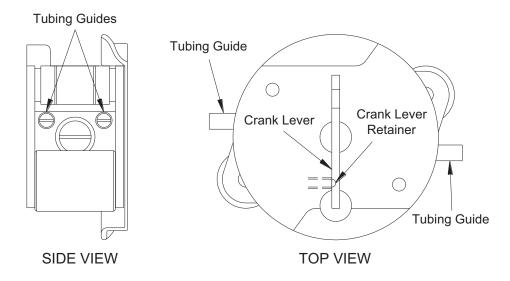



Figure 7. Blood Pump Rotor Assembly





**Note:** On newer blood pump rotors (M30990) the plastic sleeves are not replaceable. If sleeves are damaged, replace the rotor assembly.

6. On each of the tubing guides there is a plastic sleeve that should rotate smoothly. Inspect each plastic sleeve for smooth operation. If any of the plastic sleeves are missing, damaged, or do not rotate smoothly, replace with a new plastic sleeve. See Figure 8 for an exploded view and Fresenius part numbers.



Tubing Guide (Exploded View)

Figure 8. Tubing Guide (Exploded View)

7. Without removing the plastic sleeve, inspect the solid guide post on all four (4) tubing guides. The solid guide post should not be loose or bent. If any of the solid guide posts are loose or bent, the rotor assembly needs to be replaced. (Fresenius part number M30990).



**Note:** The plastic sleeve will make it feel like the solid guide post is loose. When inspecting, pay close attention to the movement of the metal shaft.



#### 2.12 FINAL CHECKS

Before returning the machine to clinical use after successful completion of all of the Preventive Maintenance procedures listed above, complete the following:

- Verify that the machine label with serial number is in place, usually on the back
  of the cabinet near the Monitor Control Unit or above the quick connectors of the
  open shunt door assembly. Record this serial number on the Preventive
  Maintenance Checklist form.
- Verify that no dialysate spills or leaks are visible in the hydraulics or on the bottom of the cabinet. Clean and dry any spills found and correct the source.
- Verify that all cables are properly routed to prevent pinching or chaffing.
- Verify that all covers are replaced and that all cover screws and mounting hardware has been replaced.



**Caution:** Reliable operation of the machine requires that all screws and covers be properly installed. Ensure that all screws and covers are in place before returning the machine to clinical use.

• Clean the exterior surfaces of the machine and remove all traces of dirt, oil or other contaminants.



**Caution:** Do not use a cleaner containing Dimethyl Benzylammonium Chloride. This ingredient will damage many plastic surfaces. Certain brands of cleaners specifically marketed to clinics and hospitals contain this ingredient. Check the contents of any unknown cleaner before using it.



#### 3.0 ANNUAL (4000 HOUR) PREVENTIVE MAINTENANCE

Perform the following Preventive Maintenance procedures every 12 months or 4000 hours of machine operation, whichever comes first. Perform the procedures in the order given below to complete the Annual Preventive Maintenance and the Quarterly Preventive Maintenance. The following procedures will refer back to the Quarterly Preventive Maintenance procedures at the proper times for you to work in the most efficient manner.

Make copies of the Annual Preventive Maintenance Checklist provided at the back of this manual and use them to record the maintenance done.

#### 3.1 FILTERS AND O-RINGS

Perform the Quarterly Preventive Maintenance procedures in Sections 2.1.

#### 3.2 PRE-UF PUMP FILTER

Replace the Pre-UF Pump Filter (Fresenius part number 672574).



**Caution:** Do not attempt to disassemble the Pre-UF Pump Filter. If not properly reassembled, the Pre-UF Pump filter may leak. A leak in the hydraulic system at this location may affect the operation of the machine or cause fluid loss from the patient.

#### 3.3 CHECK VALVES



**Caution:** Ensure each check valve is oriented correctly to allow fluid flow in the proper direction.

Replace the UF Pump Output check valves. There are two check valves at the UF pump output. One is at the UF pump itself. The other is downstream at the UF Sample Port.



#### 3.4 DEAERATION RESTRICTOR



**Note:** On newer machines with hydrochamber assemblies the deaeration restrictor is a glass bead with a fixed orifice built into one of the hydrochamber interconnecting tubes. Since there are no o-rings in this type of setup, disregard this step. If a screw is present in the back side of the hydroblock proceed with the following check.

With the machine off, replace the deaeration restrictor O-rings by clamping the hydroblock vent tube and removing the deaeration restrictor from the hydroblock (See Figure 3, pg. 8). Replace the two O-rings on the deaeration restrictor (Fresenius part number 579070). Clean any debris that may be present in the angled hole at the tip of the deaeration restrictor. Reinstall deaeration restrictor.

#### 3.5 DIASAFE® FILTER (IF APPLICABLE)

Perform the Quarterly Preventive Maintenance procedures in Sections 2.2.

#### 3.6 DIAPHRAGM PUMPS

Rebuild the UF, Bicarbonate and Concentrate diaphragm pumps as described in Section 4.1 and 4.2.



#### 3.7 HEATER ELEMENT



**Warning!** Dangerous high voltage is present at these connections when the machine is operating. The heater element is hot enough to inflict serious injury if it is touched while power is applied or shortly after power is removed. Ensure the machine is disconnected from the wall outlet.

1. Remove the rear access panels and distribution board cover so that the wires of the heater are accessable.



**Note:** If the heater element is replaced, replace the heater O-ring as well (P/N 579075).

- 2. Remove the heater element from the hydroblock on the machine (See Figure 3, pg. 8). Inspect the heater element for signs of corrosion. If corrosion exists, replace the heater element.
- 3. Attach one lead of the voltmeter to the ground (yellow / green wire) and the other lead to the brown or blue wire. Measure the resistance. Resistance should be "OL" or greater than 19.9 meg-ohms. If this is not the case, replace the heater element.
- 4. After completing this check, reinstall the heater and O-ring.

#### 3.8 HIGH VOLTAGE AC CONNECTIONS

Perform the Quarterly Preventive Maintenance procedures in Sections 2.4.



#### 3.9 DEAERATION MOTOR BRUSHES

Replace the deaeration motor brushes every 8000 hrs using the following steps:

- 1. Remove the complete deaeration motor/pump assembly from the machine.
- 2. Using a marker, make marks on the motor housing and motor cap as illustrated below. These marks will ensure the correct alignment when reassembling the motor case.

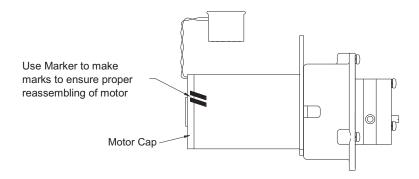


Figure 9. Deaeration Motor/Pump Assembly with marks.

- 3. Using a T-25 Torx screwdriver, remove the two screws holding the motor cap to the motor housing.
- 4. Remove the motor cap to gain access to the motor brushes. Replace the motor brushes.
- 5. Reassemble the motor, aligning the marks.
- 6. While holding the pieces together, install and tighten the two T-25 screws.



**Note:** If the motor case and motor cap are not installed using the marks, the motor will run in reverse and flow errors will result.



#### 3.10 INLET WATER PRESSURE REGULATOR

Verify that the regulator provides the proper water pressure as follows:

- 1. Shut off the water supply to the machine.
- 2. Install a gauge with a T-fitting to monitor the pressure at the outlet side of the Inlet Pressure Regulator (See Figure 3, pg. 8).



**Caution:** Use tie wraps or tubing clamps to secure the connections. The water pressure may be sufficient to blow the lines off the fittings if they are not secured.

- 3. Turn the water supply to the machine ON.
- 4. With the dialysate lines in the shunt, select Rinse Mode. The pressure gauge will cycle between two readings as water inlet valve opens and closes.



**Note:** Rinse mode causes all valves, pumps, and motors to run/activate. While in Rinse Mode inspect for any leaks; paying particular attention to areas of the hydraulics that were disassembled in previous steps during the preventive maintenance procedures.

5. Verify that the pressure gauge reads between 18 and 20psi when the pressure is at its highest value, and reads greater than 8psi when the pressure is at its lowest value.



**Note:** Readings below 8psi at the lowest level indicates inadequate inlet water flow into the machine. This may be caused by a dirty inlet filter screen or problems with the treated water supply.

- 6. Turn off the source water supply.
- 7. Turn the machine OFF, remove the gauge and reconnect the tubing using clamps to prevent leaks.
- 8. Turn the treated water supply source ON, turn the machine ON and select Dialysis Mode. Start dialysate flow and inspect all hoses and connections. Ensure that there are no leaks.



#### 3.11 ONLINE CLEARANCE TEST (IF APPLICABLE)

If the machine is equipped with Online Clearance (OLC), conduct the following test:

#### **OLC Self-Test**

1. With stable temperature and conductivity, start an OLC Self-Test by pressing the OLC Self-Test screen button on the Kt/V screen.



**Note:** Switch to the debug screens by pressing and holding the  $[\blacktriangle]$  and  $[\blacktriangledown]$  keys at the same time for approximately 1 sec. The main display will change indicating that the machine is in debug mode.

2. When the OLC Self-Test is complete, go to debug screen #5 and confirm that 0 Test (0TST prior to functional software version 3.02) is in the range ±20.



**Note:** If 0 Test (0TST) is out of range, the OLC Self-Test will fail. If this happens, conduct temperature (PRE & POST) and conductivity calibrations, then conduct OLC Self-Test again.

#### **OLC Self-Test Troubleshooting**

If the OLC Self-Test continues to fail after conducting the temperature (PRE & POST) and the conductivity calibrations, conduct the following troubleshooting steps:

1. Turn the machine ON and allow the machine to run in Dialysis Mode at 500ml/min flow rate for approximately 10 minutes. This allows the machine to come up to temperature and conductivity.



**Note:** On functional software prior to version 3.02, an OLC Self Test will start automatically as soon as temperature and conductivity are stable. Once the test starts cancel it by opening the shunt door. The cancel message will be hidden by the Shunt Door Open banner. Close the shunt door and confirm that OLC Self Test banner is gone.

2. Once the machine is warmed up, remove X3 (MON-NTC) and X7 (COND) from the distribution board.



3. Using the Resistor Plug Set for OLC Testing (Fresenius part number 190168), plug the  $6.04K\Omega$  plug into X3 (MON-NTC) and the  $274\Omega$  plug into X7 (COND) on the distribution board.



**Note:** Due to the resistor placement inside the OLC test plugs, the orientation of the plug when inserted onto the distribution board is irrelevant.

- 4. Switch to the debug screens by pressing and holding the [▲] and [▼] keys at the same time for approximately 1 sec. The main display will change indicating that the machine is in debug mode.
- 5. Use the  $[\blacktriangle]$  and  $[\blacktriangledown]$  keys to go to debug screen #5.
- 6. On debug screen #5, locate TPRE and observe its value for 1 minute. During this time, record the highest and lowest values observed in the table below.

	Highest Value	Lowest Value	Difference
TPRE		- :	=

- 7. Calculate the difference between the highest and lowest TPRE value and record it in the table above.
- 8. Verify that the difference for TPRE < 2. If the difference for TPRE > 2, then possible causes are sensor board, motor noise, or -12V problems.
- 9. Again on debug screen #5, locate CPRE and observe its value for 1 minute. During this time record the highest and lowest values observed in the table below.

	Highest Value	Lowest Value	Difference
CPRE		_ :	=

- 10. Calculate the difference between the highest and lowest CPRE value and record it in the table above.
- 11. Verify that the difference for CPRE < 8. If the difference for CPRE > 8, then possible causes are sensor board, motor noise, or -12V problems.



- 12. Remove the  $6.04K\Omega$  and  $274\Omega$  plug from the distribution board and replace the original connectors.
- 13. Remove X44 (NTC-POST) and X13 (COND-POS) from the distribution board.
- 14. Using the Resistor Plug Set for OLC Testing (Fresenius part number 190168), plug the  $6.04K\Omega$  plug into X44 (NTC-POST) and the  $274\Omega$  plug into X13 (COND-POS) on the distribution board.
- 15. On debug screen #5, locate TPOS and observe its value for 1 minute. During this time record the highest and lowest values observed in the table below.

	Highest Value	Lowest Value	Difference
TPOS		. :	=

- 16. Calculate the difference between the highest and lowest TPOS value and record it in the table above.
- 17. Verify that the difference for TPOS < 2. If the difference for TPOS > 2, then possible causes are sensor board, motor noise, or -12V problems.
- 18. Again on debug screen #5, locate CPOS and observe its value for 1 minute. During this time record the highest and lowest values observed in the table below.

	Highest Value	Lowest Value	Difference
CPOS		. :	=

- 19. Calculate the difference between the highest and lowest CPOS value and record it in the table above.
- 20. Verify that the difference for CPOS < 8. If the difference for CPOS > 8, then possible causes are sensor board, motor noise, or -12V problems.



- 21. With the  $6.04K\Omega$  plug on X44 (NTC-POST) and the  $274\Omega$  plug on X13 (COND-POS) of the distribution board, verify that CPOS does not change more then 10 increments when the dialysate flow is turned OFF. (Note: Conduct this test for the dialysate flow ON to OFF transition.)
- 22. Remove the  $6.04K\Omega$  and  $274\Omega$  plug from the distribution board and replace the original connectors.
- 23. With stable temperature and conductivity, start an OLC Self Test by pressing the OLC Self-Test screen button on the Kt/V screen.
- 24. When the OLC Self Test is complete, go to debug screen #5 and confirm that 0 Test (0TST prior to functional software version 3.02) is in the range  $\pm 20$ .



#### 3.12 DEAERATION AND LOADING PRESSURE

Verify that the deaeration pressure is between -24 and -25 inHg and the loading pressure is between 18 and 20psi (between 23 and 25psi if a DIASAFE® filter system is installed) as follows:

- 1. With dialysate flow OFF, install a gauge with a T-fitting to monitor the pressure on the inlet (suction) side of the deaeration pump (See Figure 3, pg. 8).
- 2. Connect a gauge equipped with a yellow connector into the red ACETATE/ACID port.
- 3. In Dialysis Mode, turn dialysate flow ON and verify that the gauge on the deaeration pump indicates between -24 and -25 inHg. The needle will be vibrating somewhat. Verify that it does not go higher than -24 inHg or lower than -25 Hg. Verify that the gauge in the ACETATE/ACID port indicates between 18 and 20psi (between 23 and 25psi if a DIASAFE® filter system is installed).



**Note:** When the machine is at a different elevation above sea level, it may be difficult or impossible to achieve -24inHg. The following table will help in determining the appropriate deaeration pressure calibration point at different elevations:


Elevation	Approx. atmospheric pressure	Minimum target deaeration pressure relative to atmospheric pressure
feet	mmHg	inches of Hg
0	760	-24.0
1000	728	-23.0
2000	697	-22.0
3000	667	-21.0
4000	639	-20.0
5000	612	-19.0
6000	585	-18.5
7000	561	-17.5
8000	537	-16.9
9000	514	-16.2
10000	492	-15.5



#### 3.13 FLOW RELIEF PRESSURE

Verify that the flow relief pressure is between 29 and 30psi (between 35 and 36psi if a DIASAFE® filter system is installed) as follows:

1. Turn the machine on in Service mode. From the Calibrate Hydraulics screen, select the Flow Pressure screen button. The screen will change to the following:

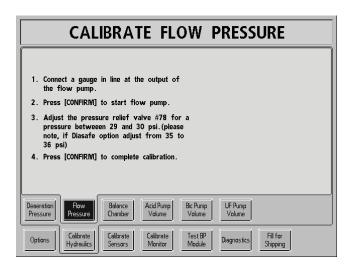

2. Connect a gauge in line at the **output** of the flow pump (See Figure 3, pg. 8).



**Note:** The output side of the flow pump is the side with the white reinforced jacket over the line. The input side has clear plastic line

- 3. Press the [CONFIRM] key to start the flow pump.
- 4. Verify the gauge indicates a pressure between 29 and 30psi (between 35 and 36psi if a DIASAFE<sup>®</sup> filter system is installed.



### 3.14 CONCENTRATE AND BICARB PUMPS

Test the Concentrate and Bicarbonate diaphragm pumps as described in Section 4.3.

#### 3.15 **UF PUMP**

Calibrate the UF Pump Volume (Refer to the 2008K Calibration Procedures – Fresenius part number 507296.)

#### 3.16 CONDUCTIVITY

Verify that the dialysate conductivity measured by the internal cell in the machine agrees with an external meter within 0.1mS/cm as described in Section 2.6.

#### 3.17 TEMPERATURE

Verify that the dialysate temperature shown on the front panel Display screen agrees with an external meter within 0.5°C at 37°C and 39°C as described in Section 2.7

#### 3.18 VOLT HI LO DETECT

Verify that the 5-volt supply is operating within 0.2 volts as reported on the debug screen as follows:

- 1. Switch to the debug screens by pressing and holding the [▲] and [▼] keys at the same time for approximately 1 sec. The main display will change indicating that the machine is in debug mode.
- 2. Use the  $[\blacktriangle]$  and  $[\blacktriangledown]$  keys to go to debug screen #4.
- 3. Locate the 5V value on the display screen. This value must be between 4.8V and 5.2V.



**Note:** If the 5V value is not within limits, the problem is most likely the 12volt supply out of tolerance. Perform the Volt Hi Lo Detect calibration procedure. Refer to the 2008K Calibration Procedures – Fresenius part number 507296.



#### 3.19 BLOOD LEAK AND DIMNESS

Verify that the blood leak level is between 4.5 and 5.2 volts and the blood dimness level is within  $5.0 \pm 1.0$  volts as follows:

- 1. Switch to the debug screens by pressing and holding the [▲] and [▼] keys at the same time for approximately 1 sec. The main display will change indicating that the machine is in debug mode.
- 2. Use the  $[\blacktriangle]$  and  $[\blacktriangledown]$  keys to go to debug screen #4.
- 3. Locate the LEAK value on the display screen. This value must be between 4.5 and 5.2.
- 4. Locate the DIMN value on the display screen. This value must be between 4.0 and 6.0.



**Note:** If these values are outside the limits given, perform a bleach rinse to clean the glass detector tube inside the machine before considering other repairs.



#### 3.20 ARTERIAL, VENOUS AND TRANSMEMBRANE PRESSURE

#### ARTERIAL PRESSURE

- 1. Inspect the internal pressure transducer protector for contamination. If contamination is found, replace the pressure transducer protector (Fresenius part number 650158) and remove and disinfect the pressure port with 1:100 bleach for a minimum of 15 minutes.
- 2. Open the arterial transducer port **P**<sub>ART</sub> on the blood pump module to air (atmospheric pressure). Verify that the **Arterial Pressure** bargraph indicates 0.
- 3. Attach a syringe and a calibrated pressure gauge to the **P**<sub>ART</sub> port using a T-fitting.
- 4. Push the syringe in to show a pressure of 200mmHg on the external gauge. Verify that the Arterial Pressure bargraph indicates 200.
- 5. Switch to the debug screens by pressing and holding the [▲] and [▼] keys at the same time for approximately 1 sec. The main display will change indicating that the machine is in debug mode.
- 6. Use the [▲] and [▼] keys to go to debug screen #1 and locate the ART value.
- 7. Increase the pressure to a range of 310 315mmHg. Clamp off the tubing at the **P**<sub>ART</sub> port and monitor the debug ART value for 30 seconds. The maximum allowable leakage is 2mmHg in 30 seconds.



#### **VENOUS PRESSURE**

- 1. Inspect the internal pressure transducer protector for contamination. If contamination is found, replace the pressure transducer protector (Fresenius part number 650158) and remove and disinfect the pressure port with 1:100 bleach for a minimum of 15 minutes.
- 2. Open the venous transducer port **P**<sub>VEN</sub> on the level detector module to air (atmospheric pressure). Verify that the **Venous Pressure** bargraph indicates 0.
- 3. Attach a syringe and a calibrated pressure gauge to the P<sub>VEN</sub> port using a T-fitting.
- 4. Push the syringe plunger in to show 400mmHg on the external pressure gauge. Verify that the Venous Pressure bargraph indicates 400.
- 5. Switch to the debug screens by pressing and holding the [▲] and [▼] keys at the same time for approximately 1 sec. The main display will change indicating that the machine is in debug mode.
- 6. Use the [▲] and [▼] keys to go to debug screen #1 and locate the VEN value.
- 7. Decrease the pressure to a range of 310 315mmHg. Clamp off the tubing at the P<sub>VEN</sub> port and monitor the debug VEN value for 30 seconds. The maximum allowable leakage is 2mmHg in 30 seconds.



#### TRANSMEMBRANE PRESSURE

- 1. With dialysate flow ON, ensure the dialysate lines are full of fluid and no air is visible passing through the flow indicator.
- 2. Hang a four-way connector to the I.V. pole at normal dialyzer height.
- 3. Set dialysate flow to 500ml/min, then press the [CONFIRM] key.
- 4. Open the arterial (**P**<sub>ART.</sub>) and venous (**P**<sub>VEN.</sub>) transducer ports to air (atmospheric pressure).
- 5. Turn the blood pump off.
- 6. Turn dialysate flow OFF, remove the dialysate lines from the shunt and attach them to the connector. Close the shunt door.



**Note:** Filling the lines before removing them from the shunt will avoid wetting the pressure gauge transducer during the test.

- 7. Connect a 30cc syringe to one of the four-way connector outlets and a pressure gauge to the remaining outlet.
- 8. Switch to the debug screens by pressing and holding the [▲] and [▼] keys at the same time for approximately 1 sec. The main display will change indicating that the machine is in debug mode.
- 9. Use the  $[\blacktriangle]$  and  $[\blacktriangledown]$  keys to go to debug screen #1.
- 10. Use the syringe to set the pressure on the external gauge to 0mmHg. Calculate the dialysate pressure measured by the machine as follows:
  - Note the value shown for TMP on the display screen.
  - Subtract the value shown for VEN on the display screen.
- 11. Verify that the calculated value is between +20 and -10mmHg.
- 12. Use the syringe to create a pressure of -250mmHg on the pressure gauge.
- 13. Calculate the dialysate pressure measured by the machine again as described in step 10. Verify that the calculated value is between 230 and -260mmHg.



#### 3.21 DIALYSATE FLOW

Verify the dialysate flow is within  $\pm 3\%$  of the stated rate at 500ml/min as follows:



**Note:** All flow rates are controlled by the software. Testing the rate at 500ml/min verifies the accuracy of all rates.

1. In Dialysis Mode, turn the dialysate flow ON at 500ml/min. Verify that the UF pump is OFF and the machine is out of bypass. Allow the dialysate flow to run for 2 minutes, minimum, before continuing.



**Note:** Do not collect the spent dialysate from the drain hose in the next step. The accuracy of the collection will be affected if not collected directly from the drain port with the drain hose removed.

2. Collect spent dialysate from the drain port on the back of the machine (See Figure 3, pg. 8) for exactly 1 minute. Verify that the amount collected is between 485 and 515ml.

#### 3.22 HEPARIN PUMP

If the machine is equipped with a heparin pump module, clean and test the pump as follows:

- Remove the heparin pump module from the machine and wipe the lower edge of the module and the heparin pump cabinet opening to remove any residual disinfecting agent.
- 2. Reinstall the heparin pump into the machine cabinet. When installing the module screws do not use a power screwdriver
- 3. Place the machine in Dialysis Mode and clear all alarms.
- 4. Select the Heparin screen button. On this screen press the Syringe button. Use the [▲] and [▼] keys to select the syringe being used for this test and press the [CONFIRM] key.
- 5. Press the Load Syringe button. Press the [CONFIRM] key and the carriage will fully retract downward.
- 6. When the carriage has stopped, press the [Escape] key and clean the carriage bar (See Figure 10).



7. Extend the syringe plunger past the 10ml mark. Install the syringe into the pump and latch the plunger handle into the carriage. If needed, squeeze the carriage/plunger release lever to slide the carriage up to meet the plunger handle. The syringe plunger should be at a position greater than 10ml.

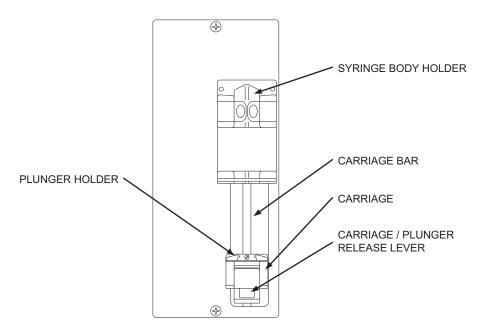


Figure 10. Heparin Pump Module.

- 8. Press the Heparin Prime button. Press and hold the [CONFIRM] key. The plunger will start moving towards the 10ml mark. Release the [CONFIRM] key as soon as the syringe plunger is aligned exactly with the 10ml mark on the side of the syringe body.
- 9. Select the Bolus data button. Use the [▲] and [▼] keys to set a value of 5.0ml then press the [CONFIRM] key.
- 10. Select the Total Infused data button. Press the 0 (zero) key and then the [CONFIRM] key.
- 11. Press the Infuse Bolus button. Press the [CONFIRM] key and start timing the interval with the stopwatch.



12. When the pump stops, use the table below to verify the time to run a 5ml Bolus is correct for the selected syringe type.

Type	Syringe Size	5ml Bolus Time
B-D	10ml	29.0 - 30.0 seconds
Terumo	10ml (12ml)	24.0 - 25.0 seconds
Monoject	10ml (12ml)	24.5 – 25.5 seconds

- 13. Also, verify that the **Total Infused** data button reads 5.0 and that the syringe plunger has moved to between 4.8 to 5.2 on the syringe scale.
- 14. Move the carriage all the way up to the end of its travel.
- 15. Select the RATE data button. Use the [▲] and [▼] keys to set a value of 9.9ml/hr then press the [CONFIRM] key.
- 16. Press the [Heparin on/off] key to start the pump. The green lamp above the key should light.
- 17. Verify that a HEPARIN PUMP ALARM is displayed on the status line within 2 minutes.



**Note:** If the machine is not alarm free, another message of higher priority may be displayed on the status line.



#### 3.23 BLOOD PUMP

Clean and test the arterial blood pump module as follows:

- 1. Remove the blood pump rotor by opening the door, pulling out the handle and turning the rotor 90 degrees
- 2. Clean the rollers with a cloth dampened only with water.
- 3. With the crank lever pulled out, locate and lubricate the crank lever retainer ball. If the crank lever is hard to pull out, replace the crank lever retainer assembly (Fresenius part number 564301).
- 4. Without removing the plastic sleeve, inspect the solid guide post on all four (4) tubing guides. The solid guide post should not be loose or bent. If any of the solid guide posts are loose or bent, the rotor assembly needs to be replaced. (Fresenius part number M30990).



**Note:** The plastic sleeve will make it feel like the solid guide post is loose. When inspecting, pay close attention to the movement of the metal shaft.

- 5. Clean the inside of the blood pump housing with the damp cloth. Compressed air may be used if it is available.
- 6. Remove the blood pump module from the machine and inspect the motor gearbox. In heavy use, some oil may accumulate on the gearbox housing. Wipe the housing clean.
- 7. Wipe the lower edge of the module and the blood pump cabinet opening to remove any residual disinfecting agent.
- 8. Reassemble the blood pump module and reinstall it in the machine cabinet. When installing the module screws do not use a power screwdriver.
- 9. Place the machine in Dialysis Mode and clear all blood alarms.
- 10. Start the blood pump if it is not already running.
- 11. Open the blood pump door. Verify that the red alarm light on the blood pump module lights within 15 or 30 seconds.



**Note:** Delay time before the blood pump alarm lights is set by dipswitch 4 on the LP955 blood pump board.



- 12. Close the blood pump door and press the [RESET] key to clear the alarm.
- 13. Test the pump as follows:
  - Set the Tubing Size to 8mm.
  - Insert a bloodline in the pump. Do not change the setting of the tubing size selector, even if you are not using 8mm tubing.
  - Connect a pressure gauge to the bloodline in the pump (See Figure 11) and allow the rotor to pull up 37°C ± 1.5°C water. Let this fluid flow past the pressure gauge long enough to clear out air.

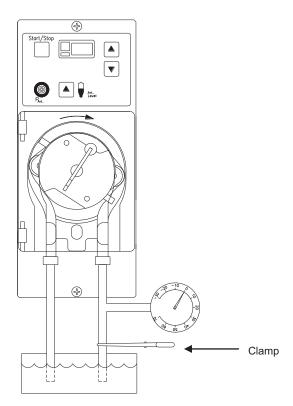


Figure 11. Blood Pump Rotor Occlusion Test

- With the pump running at 600ml/min, clamp the outlet so that the pressure gauge is between the output of the pump and the clamp (See Figure 11). The peak pressure on the gauge must be between 25 and 35psi. If the peak pressure is out of range, replace the blood pump rotor springs (Fresenius part number 650174).
- Set the Tubing Size Selector to agree with the size of bloodline used in the pump.



# 3.24 LEVEL DETECTOR

Perform the Quarterly Preventive Maintenance procedures in Section 2.8

## 3.25 ALARM AND PRESSURE HOLDING TESTS

Perform the Quarterly Preventive Maintenance procedures in Section 2.9.



#### 3.26 RINSE CHECKS

Perform the Rinse Checks as follows:

- 1. Place the machine in rinse mode, then turn the water supply off. Verify that the display screen shows NO WATER.
- 2. Turn water supply on.
- 3. Start rinse mode, and watch the flow from the drain line. The water from the drain line will stop at one point for 15 seconds. At this time put the drain line in a 1000ml graduated cylinder. Start timing when the flow starts again. At 30 seconds, remove the line from the graduated cylinder. Verify that a minimum of 310ml is collected.
- 4. To avoid problems with pre-rinse, allow the rinse to complete prior to proceeding to the next step.
- 5. Connect the dialysate lines to an external meter capable of reading at least 85°C.
- 6. Close the shunt door.
- 7. Start the machine in heat disinfect mode with the dialysate lines on the external meter as follows:
  - With the shunt door closed, reach up into the opening at the bottom of the shunt and find the two spring-loaded switches that protrude through the holes next to the connectors. Push these switches in with your fingers, simulating dialysate lines connected to the shunt.
  - While holding these switches pushed in, press the Heat Disinfect button on the startup screen.
  - While holding the switches, open the shunt door. Verify the heat disinfect does not get interrupted.
  - Leave the shunt door open; closing it will stop the heat disinfect mode.





**Warning!** Scalding hot water is passing through the dialysate lines and the external meter manifold. Allow the dialysate lines and the external meter manifold to cool before disconnecting the lines.

8. The heat disinfect timer will not be operating. It is not needed. Monitor the external temperature meter and verify that the temperature rises to between 80°C and 90°C.



**Note:** Some external temperature meters may not display correctly at higher temperatures. Consult the appropriate product literature from the meter manufacturer for applicable conversion charts.

#### 3.27 BATTERY AND POWER FAILURE ALARM

Remove the 9-volt battery located behind the monitor unit (See Figure 3, pg. 8). The battery is inside the plastic housing. Press the cover in and to the left to release it, then pull it out.



**Note:** If the 9-volt battery is swollen, the power logic board is bad and should be replaced.

With the battery removed, perform an Alarm Test and confirm the Battery Test fails.



**Note:** If the Battery Test <u>passes</u> with the 9-Volt battery removed, IC9 is bad on the Power Logic Board and should be replaced.

Replace the 9-volt battery with a new one observing the correct polarity marked inside the holder. Install the battery/holder assembly into the monitor unit.

With the new battery in place, perform an Alarm Test and confirm the Battery Test passes.

Test the power failure alarm by removing the machine power plug from the wall outlet with the machine powered on. Verify that the audible alarm sounds.



#### 3.28 BLOOD PRESSURE MODULE



**Note:** There are seven types of blood pressure modules that can be connected to the 2008K. Since each module type has different test criteria and the 2008K is unable to detect which module is connected, disregard the displayed Pass/Fail results and use the appropriate table to determine pass or fail.

Test the blood pressure module (See Figure 3, pg. 8), as follows:

Place the machine in Service Mode.

Select the Test BP Module button and the screen will change.

#### INFLATION SPEED TEST

From the Test BP Module screen, select the Inflation Speed button.

- 1. Connect the pressure tubing from the module to the 700cc port on the Test Device. Ensure the tubing fits snugly on the ports.
- 2. Press the [CONFIRM] key. The screen will change and the test will start.
- 3. The blood pressure module will pressurize the Test Device and report the time. When the test is complete, use the table below to verify that the Time to 250 value is within range dependent upon the module type installed.

Module Type	Time to 250
M400	≤ 7.3 seconds
M2000, M2600 or M3600	≤ 10.0 seconds
TM-2910 or TM-2915	≤ 10.0 seconds
SunTech	≤ 11.0 seconds

4. Press the [CONFIRM] key.



#### **DEFLATION SPEED TEST**



**Note:** The deflation speed test is not applicable to the SunTech module.

From the Test BP Module screen, select the Deflation Speed button.

- 1. Connect the pressure tubing from the module to the 220cc port on the Test Device. Ensure the tubing fits snugly on the ports.
- 2. Press the [CONFIRM] key. The screen will change and the test will start.
- 3. The blood pressure module will depressurize (deflate) the Test Device. The screen will change and report the deflation speed at various pressures in mmHg per second.
- 4. Use the table below to verify that the values reported are within the following ranges dependent upon the module type installed.

Pressure Model Type	RATE /	AT 240 g/sec)		AT 160 g/sec)	RATE (mmH	AT 80 g/sec)		AT 40 g/sec)
Woder Type	Min	Max	Min	Max	Min	Max	Min	Max
M400	4.3	6.2	4.6	6.2	3.3	5.2	2.6	4.4
M2000 or M2600	4.4	6.7	4.4	6.7	3.0	5.2	2.4	4.6
M3600	3.8	6.6	3.8	6.6	2.8	5.5	2.3	4.6
TM2910 or TM-2915	3.5	7.5	3.5	7.5	3.5	7.5	3.5	7.5
SunTech	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A

5. Press the [CONFIRM] key.

#### AIR LEAKAGE TEST

From the Test BP Module screen, select the Air Leakage button.

- 1. Connect the pressure tubing from the module to the appropriate module specific port on the Test Device (see table at the top of the next page). Ensure the tubing fits snugly on the ports.
- 2. Press the [CONFIRM] key. The screen will change and the test will start.
- 3. The blood pressure module will pressurize the Test Device as indicated by a rise in the Cuff Pressure displayed to approximately 290mmHg. An internal timer is then activated automatically. Any change in the pressure being held will show in the Cuff Pressure display.
- 4. At the end of the Air Leakage test, the pressure is automatically released, the screen will change and the Leak Rate will be displayed.



5. Use the table below to verify that the Leak Rate value is within range dependent upon the module type installed.

Module Type	Test Device Port	Leak Rate
M400, M2000 or M2600	220cc	≤15mmHg
M3600	220cc	≤12mmHg
TM-2910 or TM-2915	700cc	≤30mmHg
SunTech	700cc	≤22mmHg

#### **CALIBRATION CHECK**

#### For the M400 & TM-2910

- 1. From the Test BP Module screen, select the Calibrate Mode button.
- 2. Disconnect the pressure tube from the Test Device and connect it to a mercury manometer or similar pressure meter accurate to within ±1mmHg.
- 3. Press the [CONFIRM] key. The screen will change and the blood pressure module will pressurize the line.
- 4. When the pressure shown on the display screen and on the external meter stabilizes, verify that they agree within  $\pm 3$ mmHg.



**Caution:** Do not exceed 330mmHg in the following step. The blood pressure module may be damaged if this pressure is exceeded.

5. Over Pressure Relief Check:

Remove the hose from the external meter and connect it to a large syringe (60cc) that has its plunger pulled back. Use the syringe to over-pressurize the blood test module while watching the display carefully. Use the table below to verify that the pressure is automatically released within range dependent upon the module type installed.

Module Type	Over Pressure Release Range
M400	between 320 and 330mmHg
TM-2910	between 310 and 330mmHg



#### For the M2000 & SunTech

- 1. From the Test BP Module screen, select the Calibrate Mode button.
- 2. Disconnect the pressure tube from the Test Device and connect it to a mercury manometer or similar pressure meter accurate to within  $\pm 1$ mmHg.
- 3. Press the [CONFIRM] key. The screen will change and the blood pressure module will pressurize the line.
- 4. When the pressure shown on the display screen and on the external meter stabilizes, verify that they agree within  $\pm 3$ mmHg.
- 5. Over Pressure Relief Check:

Due to the microprocessor control of the M2000 and SunTech modules, the over pressure relief check does not need to be conducted. In fact, an over pressure relief test could permanently damage the module.

#### For the M2600 & M3600

- 1. From the Test BP Module screen, select the Air Leakage button.
- 2. Disconnect the pressure tube from the Test Device and connect it to a mercury manometer or similar pressure meter accurate to within ±1mmHg.
- 3. Press the [CONFIRM] key. The screen will change and the blood pressure module will pressurize the line.
- 4. The blood pressure module will pressurize as indicated by a rise in the Cuff Pressure displayed to approximately 290mmHg. An internal timer is then activated automatically.
- 5. When the pressure shown on the display screen and on the external meter stabilizes, verify that they agree within ±3mmHg.
- 6. At the end of the Air Leakage test, the pressure is automatically released.
- 7. Over Pressure Relief Check:
  - Due to the microprocessor control of the M2600 and M3600, the over pressure relief check does not need to be conducted. In fact, an over pressure relief test could permanently damage the module.



#### For the TM-2915

- 1. From the Test BP Module screen, select the Air Leakage button.
- 2. Disconnect the pressure tube from the Test Device and connect it to a mercury manometer or similar pressure meter accurate to within 1mmHg.
- 3. Press the CONFIRM key. The screen will change and the blood pressure module will pressurize the line.
- 4. The blood pressure module will pressurize as indicated by a rise in the Cuff Pressure displayed to approximately 290mmHg. An internal timer is then activated automatically.
- 5. When the pressure shown on the display screen and on the external meter stabilizes, verify that they agree within 3mmHg.
- 6. At the end of the Air Leakage test, the pressure is automatically released.
- 7. Press the CONFIRM key.



**Caution:** Do not exceed 330mmHg in the following step. The blood pressure module may be damaged if this pressure is exceeded.

#### Over Pressure Relief Check:

- 8. Remove the hose from the external meter and connect it to a large syringe (60cc) that has its plunger pulled back.
- 9. From the Test BP Module screen, select the Calibrate Mode button.
- 10. From the first Calibrate Mode screen, press the CONFIRM key.

  Use the syringe to over-pressurize the blood pressure module while watching the display carefully. Verify that the pressure is automatically released between 310 and 330mmHg.

#### 3.29 FINAL CHECKS

- 1. Check the machine for any optional components that are not included here. Perform the preventive maintenance tests provided with those units.
- 2. Perform the Quarterly Preventive Maintenance procedures in Section 2.11.



#### 4.0 REBUILDING THE DIAPHRAGM PUMPS

The machine contains two types of diaphragm pumps. The ultrafiltration (UF) pump is a solenoid coil type. The concentrate and bicarbonate pumps are stepper motor types.

### 4.1 REBUILDING THE ULTRAFILTRATION PUMP

Figure 12 shows an exploded view of the ultrafiltration pump. When working on the pump, be especially careful to do the following:

- Do not lose the wear button or the shim washers inside the pump solenoid.
- Count the shim washers when you disassemble the pump. The number of washers varies as needed to mate the solenoid to the pump properly.



**Caution:** Replace exactly the same number of shims in the ultrafiltration pump as were removed. The pump will not operate correctly if the same number of shims are not replaced.

Examine all components for signs of corrosion. Replace any components that show signs of excessive rust.



**Note:** If the UF pump does not provide output even though the green light is on and not flashing, inspect the check valves. If a check valve is installed backwards, the pump will not work.



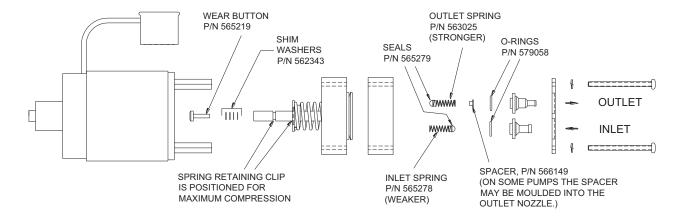


Figure 12. Ultrafiltration Pump Exploded View.

Rebuild the ultrafiltration pump as follows:

- 1. Remove the UF pump from the machine (See Figure 3, pg. 8). Make a note of which line goes to which port on the pump. When looking at the end plate, the arrow pointing into the pump nozzle is the input side. The arrow pointing away from the pump nozzle is the output side.
- 2. Hold the two sections of the pump housing and end plate together with one hand and remove the four long screws from the end plate.
- 3. Carefully remove the end plate to reveal the input and output nozzles, springs, seals and O-rings.
- 4. Replace the inlet and outlet springs.



**Caution:** Be certain the correct springs are used. The weaker spring goes on the inlet side. The stronger spring goes on the outlet side.

- 5. Inspect the seals. Replace them if there is any sign of swelling or wear.
- 6. Inspect the O-rings. Replace them if there is any sign of wear.






**Note:** Before reassembling the UF pump, verify nothing has fallen into the solenoid opening.

- 7. Reassemble the pump as follows:
  - The outlet seal goes toward the pump membrane.
  - The inlet seal faces away from the pump membrane.
  - Reinstall the spacer in the outlet nozzle if one was removed from the pump.
  - Ensure the outlet nozzle is oriented so it will be at the top of the pump solenoid to help avoid air locks in the pump.
- 8. Replace the long screws into the end plate and tighten.
- 9. Replace the pump in the machine and reconnect the electrical and hydraulic lines. Orient the pump so the outlet nozzle is above the inlet nozzle to help avoid air locks.
- 10. To displace air and to check for leaks, start a rinse and allow the machine to complete the entire rinse cycle.
- 11. Verify proper function of the UF pump by performing the Quarterly Preventive Maintenance procedure in Section 2.5.



#### 4.2 REBUILDING THE CONCENTRATE AND BICARBONATE PUMPS

Figure 13 is an exploded view of the concentrate and bicarbonate pumps.

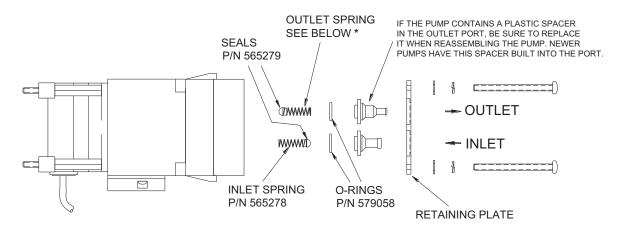

\* ON CONCENTRATE (ACID) PUMPS THIS SPRING IS STRONGER THAN THE INLET SPRING. USE P/N 563025. ON BICARBONATE PUMPS USE WEAK SPRINGS FOR BOTH INLET AND OUTLET (P/N 565278).

ON MACHINES WITH ONLINE CLEARANCE (OLC), THE CONCENTRATE (ACID) PUMP USES WEAK SPRINGS FOR BOTH INLET AND OUTLET (P/N 565278).

Figure 13. Concentrate and Bicarbonate Pump Exploded View.

Rebuild the concentrate pumps as follows:

- 1. Remove the pump from the machine (See Figure 3, pg. 8). Make a note of which line goes to which port on the pump. When looking at the end plate, the arrow pointing into the pump nozzle is the input side. The arrow pointing away from the pump nozzle is the output side.
- Hold the two sections of the pump housing and end plate together with one hand and remove the long screws that hold the end plate. On some models of the pump, all four screws hold the end plate, and on others only two screws hold the end plate.

If you removed all four screws to free the end plate, replace one or two of them to avoid having the pump come completely apart. You only need access to the inlet seals and springs.



- 3. Carefully remove the end plate to reveal the input and output nozzles, springs, seals and O-rings.
- 4. Replace the inlet and outlet springs.



**Caution:** Be certain the correct springs are used on concentrate pumps. See Figure 13 on previous page.

- 5. Inspect the seals. Replace them if there is any sign of swelling or wear.
- 6. Inspect the O-rings. Replace them if there is any sign of wear.
- 7. Reassemble the pump as follows:
  - The outlet seal goes toward the pump membrane.
  - The inlet seal faces away from the pump membrane.
  - Reinstall the spacer in the outlet nozzle if one was removed from the pump.
  - Ensure the outlet nozzle is oriented so it will be at the top of the pump solenoid to help avoid air locks in the pump.
- 8. Replace the long screws into the end plate and tighten.
- 9. Replace the pump in the machine and reconnect the electrical and hydraulic lines. Orient the pump so the outlet nozzle is above the inlet nozzle to help avoid air locks.
- 10. To displace air and to check for leaks, start a rinse and allow the machine to complete the entire rinse cycle.
- 11. Test the rebuilt diaphragm pump by performing the procedure described in Section 4.3.



#### 4.3 TESTING CONCENTRATE AND BICARBONATE PUMPS

The concentrate (acid) and bicarbonate pumps are tested by measuring the volume of water they pump and comparing that measurement with the expected value determined by the machine. The measured pump volume must be within 2% of the expected value.

Test each pump as follows:

- 1. Place the machine in Dialysis Mode and clear all alarms.
- 2. Switch to the debug screens by pressing and holding the [▲] and [▼] keys at the same time for approximately 1 sec. The main display will change indicating that the machine is in debug mode.
- 3. Use the  $[\blacktriangle]$  and  $[\blacktriangledown]$  keys to go to debug screen #1.
  - Locate the debug value for FILACT. In order to turn off dialysis flow later, FILACT must be 0.
  - Locate the debug value for DOUBLE. Certain types of Bicarbonate or higher Bicarbonate levels selected will require the pump to double stroke. If the debug value for DOUBLE is 1, the pump is double stroking. Before continuing the test, adjust the Bicarbonate level until the debug value for DOUBLE is 0.
  - If the debug values for the Bicarbonate Pump Volume (BMIN and BMAX) are showing 0 on debug screen #1, the machine is set up for a concentrate family that does not use bicarbonate. Change the concentrate selection to one requiring bicarbonate.



**Note:** The AMIN, AMAX, BMIN, BMAX are the expected limits for twenty pulses of the acid (concentrate) pump volume and the bicarbonate pump volume, respectively. These volumes are based on the measured volume of the balancing chamber to produce the correct mixing ratio.

- 4. Press the [Dialysate Flow on/off] key to stop dialysate flow.
- 5. Connect a 25ml buret filled with water to the concentrate connector for the pump to be tested. Use a short length of tubing forced over the end of the connector, and make sure there are no leaks in the fitting to the connector or to the buret.



6. With the machine in Dialysis Mode, press the [Dialysate Flow on/off] key to start the flow. Observe that liquid is drawn from the buret in discrete steps. Allow the machine to run and pump fluid from the buret for about 20 strokes, to prime the pump. Press the [Dialysate Flow on/off] key to stop the flow.



**Note:** Do not let the buret run dry so that air can enter the system.

- 7. Refill the buret exactly to the full mark. Press the [Dialysate Flow on/off] key to start the flow and count exactly 20 pulses of water drawn from the buret, then stop the flow.
- 8. Measure the amount of water drawn from the buret carefully to within 0.05ml (within 1/2 division on a buret calibrated in 0.1ml increments). Verify that this value is between the displayed limits of AMIN and AMAX for the acid pump volume and BMIN and BMAX for the bicarbonate pump volume.
- 9. If a pump volume falls outside of the permitted error, repeat the above procedure to ensure that you are getting consistent results before recalibrating the machine.



NOTES:		
	 · · · · · · · · · · · · · · · · · · ·	 
	 · · · · · · · · · · · · · · · · · · ·	 
	 · · · · · · · · · · · · · · · · · · ·	 

<b>V</b> NOTES:				
	<del></del>	 	· · · · · · · · · · · · · · · · · · ·	 
	<del> </del>	 	· · · · · · · · · · · · · · · · · · ·	 



# PREVENTIVE MAINTENANCE CHECKLIST QUARTERLY/1000 HOUR

SERIAL N	01	DATE
		MACHINE HOURS
		LABOR HOURS
	the Referenced Section of the Fresenius 2008K Preventive Senius part number 507297 Rev H) for detailed instructions	
Ref. Sect	<u>ion</u> <u>Procedure</u>	Completed By:
2.1	Clean Filters (replace if necessary) and replace O-Ring	
	Water Inlet	
	Acid and Bicarbonate Connectors	
	Dialysate Inline Filter  Dialysate Line Connectors	
	Inspect Pre-UF Pump (replace if necessary)	
2.2	Replace DIASAFE® filter (If Applicable)	
2.3	Inspect UF Pump Check Valves (replace if necessary).	
2.4	Check High Voltage AC Connections	·····
2.5	Calibrate UF Pump	·····
2.6	Check Conductivity with External Meter	······
2.7	Check Temperature with External Meter	·····
2.8	Check and Calibrate Level Detector	·····
2.9	Check Alarm Operation and Pressure Holding Test	······
2.10	Check Power Failure Alarm	·····
2.11	Inspect Blood Pump Rotor	······
2.12	Final Checks	
NOTES:		

NOTES:		



# PREVENTIVE MAINTENANCE CHECKLIST ANNUAL/4000 HOUR

SERIAL NO.	DATE
MACHINE I.D. NO	MACHINE HOURS
TECHNICIAN(S)	LABOR HOURS

See the Referenced Section of the Fresenius 2008K Preventive Maintenance Procedures (Fresenius part number 507297 Rev H) for detailed instructions to perform the following:

`	enius part number 50/29/ Rev H) for detailed instructions to perform t	2
Ref. Secti	<del></del>	Completed By:
3.1	Clean Filters and Replace O-Rings	
3.2	Replace Pre-UF Pump Filter	
3.3	Replace UF Pump Check Valves	
3.4	Check Deaeration Restrictor and Replace O-Rings	
3.5	Replace DIASAFE® filter (If Applicable)	
3.6	Rebuild UF, Concentrate and Bicarbonate Pumps	
3.7	Check Heater Element	
3.8	Check High Voltage AC Connections	
3.9	Replace Deaeration Motor Brushes (every 8000 hrs)	
3.10	Check Inlet Water Pressure Regulator	
3.11	Conduct Online Clearance Test (If Applicable)	
3.12	Check Deaeration and Loading Pressure	
3.13	Check Flow Relief Pressure	
3.14	Test Concentrate and Bicarbonate Pumps	
3.15	Calibrate UF Pump	
3.16	Check Conductivity Calibration	
3.17	Check Temperature Calibration	
3.18	Check Volt Hi Lo Detect	
3.19	Check Blood Leak and Dimness Calibration	
3.20	Check Arterial, Venous and TMP Calibration	
3.21	Check Dialysate Flow	
3.22	Check Heparin Pump (If Present)	
3.23	Check Blood Pump	
3.24	Check and Calibrate Level Detector	
3.25	Check Alarm and Pressure Holding Tests	
3.26	Rinse Checks	
3.27	Replace Battery and Check Power Failure Alarm	
3.28	Check Blood Pressure Module	
3.29	Final Checks	

7			
OTES:			
	 	 · · · · · · · · · · · · · · · · · · ·	
	 	 · · · · · · · · · · · · · · · · · · ·	

# **COMMON CONVERSIONS**

# **PRESSURE**

1 Bar	29.53 inHg
1 inHg	25.4 mmHg
1 Psi	51.72 mmHg


# **VOLUME**

1 FLUID OUNCE	26.6 MILLILITERS	
1 U.S QUART	0.946 LITERS	
1 U.S. GALLON	3.8 LITERS	
0.034 FLUID OUNCES	1 MILLILITER	
1.057 QUARTS	1 LITER	
0.26 U.S. GALLON	1 LITER	

# **MASS**

1 OUNCE (avdp.)	28.35 GRAMS
1 POUND (avdp.)	0.45 KILOGRAM
0.035 OUNCE (avdp.)	1 GRAM



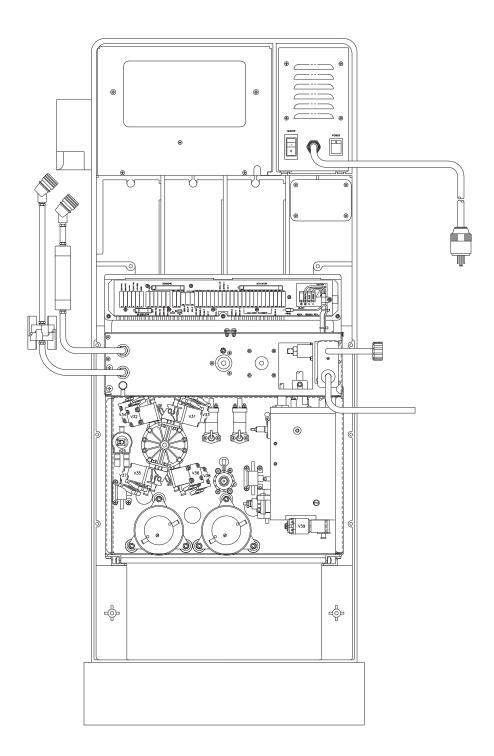

#### **Fresenius Medical Care North America**

Manufactured by: Fresenius USA, Inc. 2637 Shadelands Drive Walnut Creek, CA 94598 800 227-2572

http://www.fmcna.com