



SERVICE BULLETIN

KODAK X-OMAT Processor

Eastman Kodak Company/Customer & Technical Services/Health Sciences Markets Division/Rochester, New York 14650

SERVICE BULLETIN NO. 210

October 1994

Kodak M35, M35A, M35-M and M35A-M X-Omat PROCESSORS Kodak Industrex PROCESSORS, Models M35 and M35-A

Modification to the DETECTOR CROSSOVER ASSEMBLIES

Starting in October 1994, the M35 Series PROCESSORS with the following serial numbers will have a different DETECTOR CROSSOVER ASSEMBLY, Part No. 5B6163.


<i>Kodak PROCESSOR</i>	Serial Number
<i>M35 X-Omat</i>	39100 and higher
<i>M35A X-Omat</i>	13200 and higher
<i>M35A-M X-Omat</i>	52100 and higher
<i>M35-M X-Omat</i>	76000 and higher
<i>Industrex, Model M35</i>	95030 and higher
<i>Industrex, Model M35-A</i>	85030 and higher

- The DETECTOR DRIVE ROLLER and the DETECTOR DRIVEN ROLLER have been interchanged. The new part numbers are as follows:
 - DETECTOR DRIVE ROLLER - 246882
 - DETECTOR DRIVEN ROLLER - 246883
- A new TIE ROD **5B6150** will replace the existing TIE ROD 287035 and will allow more clearance between the FLANGE on the DETECTOR DRIVEN ROLLER 246883 and the TIE ROD.

See the figure on the back page of this service bulletin.

IMPORTANT

Do not install DETECTOR CROSSOVER ASSEMBLIES 333794, made for PROCESSORS manufactured before October 1994, in PROCESSORS with serial numbers higher than those in the table above. The new DETECTOR CROSSOVER ASSEMBLY 5B6163 is adaptable to all M35 Series PROCESSORS.

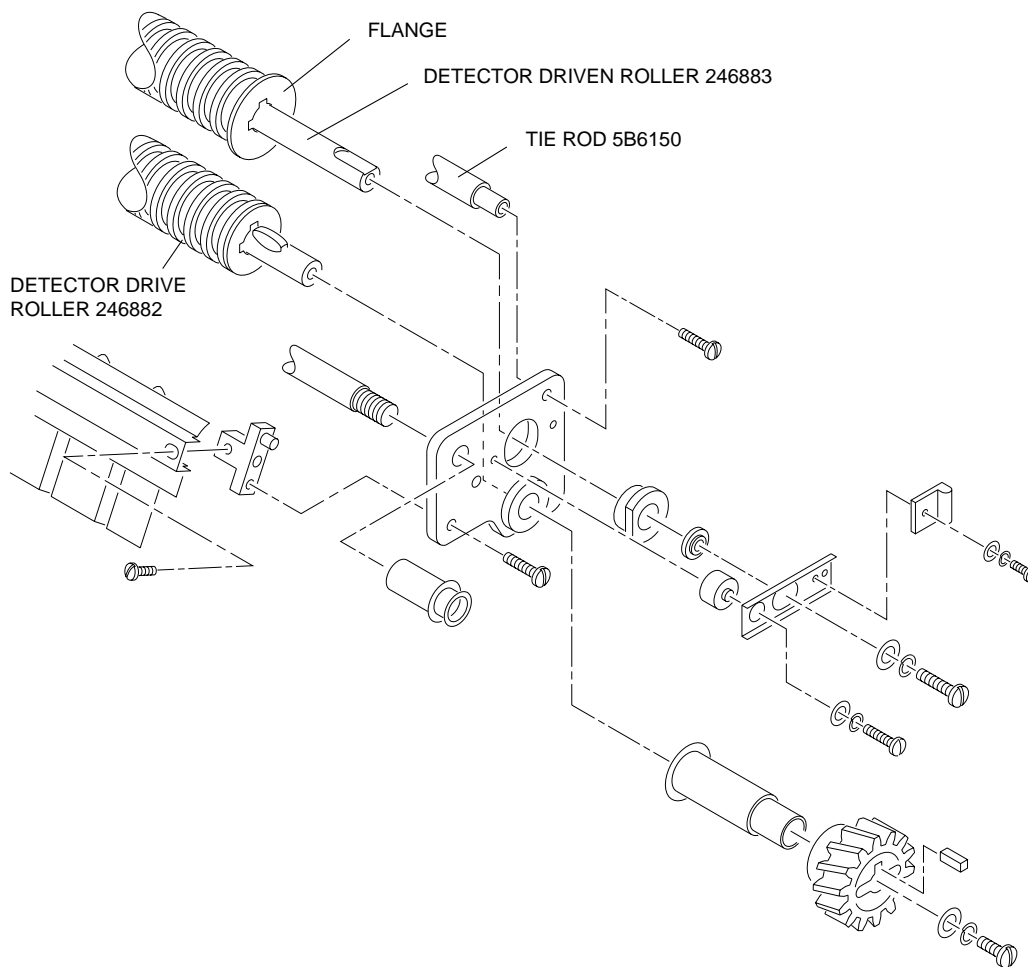

H112_0205DCA
H112_0205DA

New DETECTOR CROSSOVER ASSEMBLY 5B6163

For more information, please contact:

Eastman Kodak Company
Imaging Service Center
Health Sciences Division
100 Carlson Road
Rochester, New York 14653-9013 (716) 724-1789, Option 1

Please be prepared to give your Service Customer Number and your equipment serial number.

svcbul_210txt
N-922

Kodak, Industrex, and X-Omat are trademarks.

